

1-1-2003

Spectrum Visualization and Measurement of Power Parameters of Microwave Wideband Noise

Marina Koledintseva
Missouri University of Science and Technology

Alexander A. Kitaytsev

V.A. Konkin

V. Radchenko

Follow this and additional works at: http://scholarsmine.mst.edu/ele_comeng_facwork



Part of the [Electrical and Computer Engineering Commons](#)

Recommended Citation

M. Koledintseva et al., "Spectrum Visualization and Measurement of Power Parameters of Microwave Wideband Noise," *Proceedings of the 20th IEEE Instrumentation and Measurement Technology Conference, 2003. IMTC '03*, Institute of Electrical and Electronics Engineers (IEEE), Jan 2003.

The definitive version is available at <https://doi.org/10.1109/IMTC.2003.1207948>

This Article - Conference proceedings is brought to you for free and open access by Scholars' Mine. It has been accepted for inclusion in Electrical and Computer Engineering Faculty Research & Creative Works by an authorized administrator of Scholars' Mine. This work is protected by U. S. Copyright Law. Unauthorized use including reproduction for redistribution requires the permission of the copyright holder. For more information, please contact scholarsmine@mst.edu.

Spectrum Visualization and Measurement of Power Parameters of Microwave Wideband Noise

Marina Koledintseva

EMC Laboratory, Electrical and Computer Engineering Department, University of Missouri-Rolla
Miner Circle, 1870, Rolla, MO, 65401, USA

Phone: +1-573-341-6659, Fax: +1-573-341-4532, E-mail: marinak@ece.umr.edu

Alexander Kitaitsev, Vsevolod Konkin, Vladimir Radchenko

Department of Gyromagnetic Radio Electronics, Institute for Radio Engineering and Electronics, Moscow Power Engineering
Institute (Technical University)

Kransokazarmennaya St., 14, Moscow 111250, Russia

Phone: +7-095-362-7958, E-mail: kitaitsev@MPEI-14.MPEI.ac.ru

Abstract – A method for an adequate visualization of a microwave intense noise envelope in a wide frequency range (several octaves), measuring of its power parameters, and detection of a narrowband signal with unknown frequency and power against the noise background is presented. This method is based on an application of a non-heterodyne principle of microwave frequency (and power) conversion using a gyromagnetic converter, which operates in two regimes in turn: the resonance detection and the cross-multiplication. A block-scheme and an operation of a two-channel measuring device combining the mentioned functions are discussed.

I. INTRODUCTION

An adequate visualization of wide-band microwave spectra (up to several octaves), as well as measuring of their parameters is an actual problem at the design, testing, and practical application of microwave active devices, such as oscillators, amplifiers, active mixers, etc., especially those of high and middle power levels [1].

The method and the device for its realization presented herein combine several functions. The first one is the reproduction and visualization of a wideband random signal (in this paper it will be referred as “noise”) spectrum envelope. The second function is the measuring of the wideband noise spectrum power parameters, such as spectral power density, integral power in the chosen frequency range, spectrum bandwidth, and its central frequency. The third function is the detection, identification, and measuring of narrowband deterministic signals that might be present in the spectrum of a random signal.

Standard spectrum analyzers for microwave frequencies usually use heterodyne principle of frequency conversion. To identify numerous channels of reception, expensive high-quality microwave preselectors, complicated calibration techniques, and cumbersome computer processing are required. The difficulties increase when a source of radiation is unmatched with the input of an analyzer, or when radiation from several sources must be analyzed simultaneously. Problems occur also at using broadband power meters with a

set of parallel filters at the input, because of the necessity of matching them with the radiation sources over all the broad frequency range. Besides, the dynamic range of microwave detectors is limited, and this does not allow, for example, measuring noise spectrum power parameters in the presence of an intense interference.

The *Measurer of Spectrum Power Density (MSPD)*, the block-scheme of which is shown in Fig. 1, was developed in MPEI (TU) [2,3], and it is free from the shortcomings mentioned above.

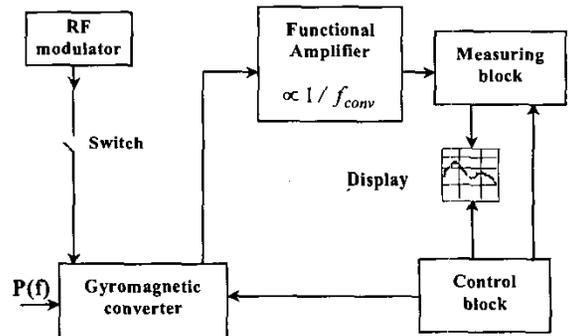


Fig. 1. Block-scheme of the measurer of spectrum power density.

The MSPD contains a gyromagnetic converter (GC). As shown in Fig. 2, the GC is a section of a transmission line (usually, coaxial or stripline), containing a high-Q monocrystalline ferrite resonator on a dielectric base. The ferrite resonator is surrounded in its equatorial plane by a microcoil, which is a planar spiral coil of about 20-25 turns made of a wire having a diameter of several dozens micrometers. This microcoil is used for both an RF modulation of the ferrite resonance frequency and getting an induced voltage due to an interaction of the ferrite resonator with a microwave magnetic field. The transmission line is placed into an electromagnet for the ferrite saturation and periodical linear varying of its resonance frequency for frequency scanning in the range of the spectrum analysis.

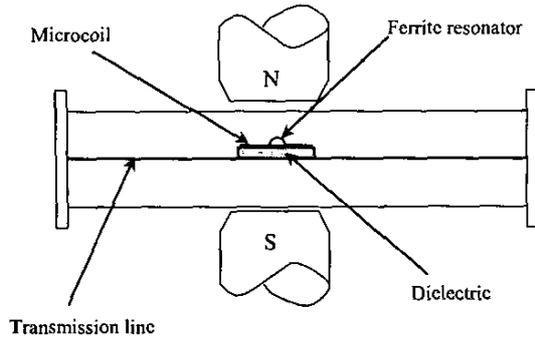


Fig. 2. Schematic of a gyromagnetic converter.

The principle of the GC operation is based on stable nonlinear resonance effects (SNLRE's) at ferromagnetic resonance (FMR), when microwave power is lower than spin-wave instability level [1,4]. There are two possible regimes of the GC operation. First is the resonance detection (RD), when there is no RF modulation of the ferrite resonance frequency, and the second is the cross-multiplication (CM), when the resonance frequency is modulated by an RF oscillation [1,2]. The typical operating frequency range of the MSPD starts from 300 MHz, and depending on the design of the GC can be up to several dozen of GHz. The GC pass-band Δf_{GC} , which determines the MSPD frequency resolution, is usually units of MHz. The range of spectrum power density that can be measured is 0.1-100 W/MHz. The own linear dynamic range of a GC is about 25 dB [2]. Due to the frequency-selectivity of the GC, the non-heterodyne frequency conversion, and stability at the microwave power overload, the MSPD allows: measuring high-intensity noise power density in the given frequency band, central frequency of the spectrum, and integral noise power [3].

The MSPD operates as follows. When measurements are conducted, the GC is used at the resonance detection regime (without the RF modulation). The RF modulation in the GC of the MSPD is used only for calibration purposes of the device, and after the calibration is accomplished, it is switched off. Part of the spectrum of a microwave wideband random (noise) signal falls into the FR resonance line and causes both precession and nutation of the ferrite magnetization vector, so that there is a variation of the longitudinal component of the magnetization vector M_z .

The behavior of the magnetization vector of the FR is described by the equation of motion with a dissipative term in one of the forms, for example, the modified Bloch's form [5],

$$\frac{d\vec{M}}{dt} = -\mu_0\gamma[\vec{M} \times \vec{H}] + \frac{\omega_r}{\mu_0}(\chi_0\vec{H} - \mu_0\vec{M}), \quad (1)$$

where \vec{H} is a total effective magnetic field acting on the magnetic moment \vec{M} ; $\mu_0 = 4\pi \cdot 10^{-7}$ H/m is permeability of vacuum; $\gamma = 1.76 \cdot 10^{11}$ C/kg is a gyromagnetic ratio; χ_0 is the

static magnetic susceptibility; and ω_r is the relaxation frequency. Assuming that the ferrite is magnetized by the magnetic field H_{0z} along the z-axis, and the microwave magnetic field has only transversal $h_{x,y}$ components, at the small angles of the magnetization vector precession, the longitudinal component M_z is related to the transversal microwave components of magnetization vector m_x and m_y by a square-law equation [5],

$$M_z(t) = M_0 - \frac{1}{2M_0}(m_x^2(t) + m_y^2(t)), \quad (2)$$

where M_0 is the equilibrium magnetization amplitude, which coincides with the saturation magnetization M_s for ferrites with low internal field of magnetic crystallographic anisotropy, e.g. ferrogarnets. The transversal components of magnetization vector are found from the FR external magnetic susceptibility tensor equation in frequency domain [5],

$$\vec{m}(\omega) = \vec{\chi}_m^{ext}(\omega) \cdot \vec{h}(\omega), \quad (3)$$

where $\vec{h}(\omega) = h_x(\omega)\vec{x}^0 + h_y(\omega)\vec{y}^0$ is the transversal microwave magnetic field, and $\omega = 2\pi f$.

The resulting magnetic flux variation due to variation of the longitudinal component of magnetization vector, induces a voltage in the microcoil,

$$V(t) = k \frac{dM_z}{dt}, \quad (4)$$

where the coefficient k depends on the geometry and the parameters of microcoil wire. The spectrum of the voltage (4) in the microcoil is

$$|V(\omega_{conv})| = \omega_{conv} k F(\omega_{conv}), \quad (5)$$

where $F(\omega_{conv})$ is the spectrum of the longitudinal component M_z at "low" frequencies of the converted signal $\omega_{conv} = 2\pi f_{conv}$.

The converted spectrum (5) is then processed by a wideband functional amplifier (see Fig.1) with special amplitude-frequency characteristic $|K(f_{conv})| = K_0 / f_{conv}$ to provide proportionality of the input spectrum power density at every frequency to the converted signal spectrum for adequate reproduction of the spectrum envelope.

Sometimes narrowband deterministic signals are present at the background of a noise signal. For a number of EMI/EMC applications it is important to tell these signals from the noise spectrum envelope inhomogeneities, which are of a random origin, and also identify their intensity and frequency. However, the MSPD cannot do this.

II. PROPOSED MEASURING METHOD AND DEVICE FOR ITS REALIZATION

A method presented herein allows combining both measurement of the noise spectrum power parameters and detecting narrowband deterministic signals against the noise background. The principle of this is based on physical properties of ferrite resonators used in the GC at the interaction of a ferrite resonator with microwave electromagnetic field, and the redistribution of the converted spectrum, when the RF modulation of the ferrite resonance frequency is switched on and off. A two-channel measuring device for this method realization broadens the possibilities of the MSPD [7]. The block-scheme of the two-channel measuring device (TCMD) is presented in Fig. 3.

In this device, the regime of the GC operation is periodically switched from the resonance detection to cross-multiplication, and the spectrum envelopes obtained in two regimes are compared. The presence of modulation in cross-multiplication regime "underlines" the deterministic signal components if they are present at the background of the wideband random noise signal [7]. This is due to the signal and noise redistribution in the spectrum of the converted signal when modulation is introduced. At the cross-multiplication regime, the total magnetization field contains a "constant" component \vec{H}_{0z} (which is actually changed with a "saw" law because of the resonance frequency slow tuning in the range of observation), and an RF modulation part,

$$H_z = H_{0z} + h_{mod z} \cdot \cos(\Omega t + \varphi). \quad (6)$$

Spectrum of the variation of the longitudinal component of magnetization vector ΔM_z , when the microwave signal with the magnetic field amplitude $h_m(\omega) = \sqrt{h_x^2 + h_y^2}$ acts on the FR, is [8]

$$\Delta M_z = \omega_M^2 h_m^2 \frac{1}{8M_S \delta^2} \times \left(\Psi_0(a, p, q) + \sum_{n=1}^{\infty} \Psi_n(a, p, q) \cos(n\Omega t - \varphi_n) \right), \quad (7)$$

where M_S is the saturation magnetization; δ is a half of the FR resonance line width at the level of -3 dB; $\omega_M = \mu_0 \gamma M_S$. Functions $\Psi_n(a, p, q)$ are the normalized harmonics of the longitudinal component of magnetization, and $\varphi_n = \varphi_n(a, p, q)$ are the corresponding phases of the harmonics [8,9]. These harmonics depend on the relative detuning of the ferrite resonator

$$a = \frac{\omega - \omega_0}{\delta}; \quad (8)$$

the normalized magnetic field amplitude of modulation for the GC

$$q = \frac{\mu_0 \cdot \gamma \cdot h_{mod z}}{\Omega}; \quad (9)$$

and the relative modulation frequency

$$p = \frac{\Omega}{\delta} = \frac{2f_{mod}}{\Delta f_{GC}}, \quad (10)$$

where $\delta = \pi \Delta f_{GC}$, $\Omega = 2\pi f_{mod}$.

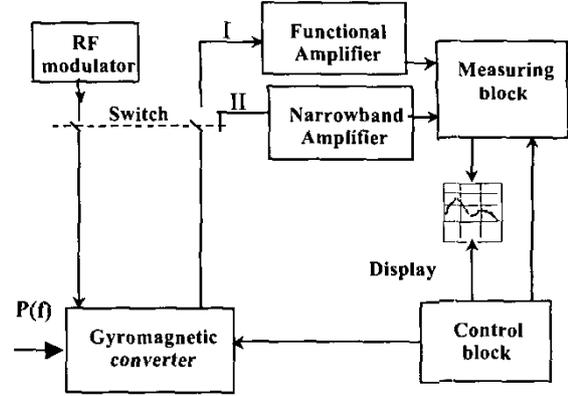


Fig. 3. Block-scheme of the two-channel measuring device.

Fig. 4 illustrates physics of interaction of the microwave signal with a FR at modulation of its resonance frequency. The longitudinal component M_z of magnetization vector varies in time when the additive sum of a random and deterministic signals act on the ferrite resonator in the vicinity of its resonance frequency, and a voltage is induced in the microcoil.

Power spectral density of the converted noise is found using the correlation theory of normal stationary random processes and Weiner-Khinchine theorem [6]. According to (2), the longitudinal component of magnetization ΔM_z is related to the squares of transversal components $m_{x,y}(t)$, which are normal random processes if the microwave noise $h(t)$ is a normal random stationary process. If an additive sum of a noise and a deterministic microwave signal ("signal + noise") acts on the GC operating in the GC regime, then there are two terms in the converted energy spectrum, due to "noise" and "signal and noise" beatings, and these parts of the spectrum are both continuous [10],

$$F_{RD}(\omega_{conv}) = F_N(\omega_{conv}) + F_{SN}(\omega_{conv}); \quad (11)$$

$$F_N(\omega_{conv}) = \frac{2\delta k^2 (\sigma_x^2 + \sigma_y^2)}{M_0^2} \cdot \frac{\omega_{conv}^2}{(2\delta)^2 + \omega_{conv}^2}; \quad (12)$$

$$F_{SN}(\Omega) = \frac{\delta k^2 (\sigma_x^2 + \sigma_y^2)}{M_0^2} \cdot P(\omega) \cdot \left(\frac{\omega_M}{2\delta} \right)^2 \frac{\omega_{conv}^2}{\delta^2 + \omega_{conv}^2}. \quad (13)$$

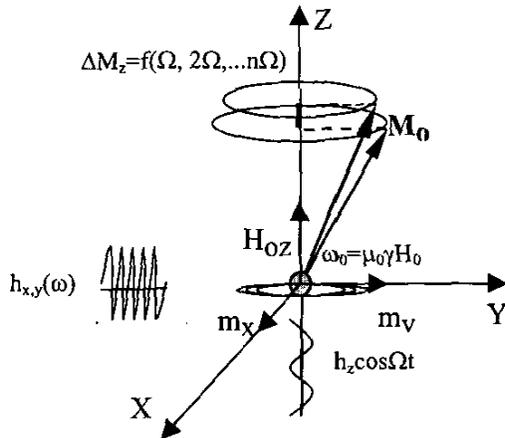


Fig. 4. Interaction of microwave signal with the ferrite resonator at modulation of its resonance frequency

At the CM regime, when the modulation is introduced into a spiral microcoil of the GC, the discrete deterministic signal energy spectrum is added,

$$F_{CM}(\omega_{conv}) = F_N(\omega_{conv}) + F_{SN}(\omega_{conv}) + F_S(n\Omega). \quad (14)$$

where $F_S(n\Omega)$ is found from (7). The first two terms in (14) are the same as in (11), since modulation in the microcoil does not affect the variation of the longitudinal component of magnetization vector associated with a random signal or beating "signal and noise". Fig. 5 shows continuous and discrete components of the ΔM_z spectrum at comparatively low frequencies of the converted signal ω_{conv} . Thus, when the RF modulation at the CM regime is present, the signal-to-noise ratio increases compared to the RD case. As a result, the envelopes of the same converted noise spectrum containing the narrowband signal at the CM and RD regimes differ, and Fig. 6 illustrates this.

The principle of the deterministic signals detection on the background of wideband microwave noise is based on this difference of spectrum envelopes [7]. The corresponding two-channel device for this method implementation shown in Fig. 3 was realized on the basis of the panoramic MSPD described in Section I. The first (*Measuring*) channel containing a wide-band functional amplifier works only when the GC operates in the RD regime. The second (*Detecting*) channel contains a narrow-band amplifier, for example, with central frequency tuned at the second harmonic of the modulation signal frequency. The modulator is an oscillator with high stability of its frequency typically chosen at several MHz. The low-pass and high-pass filters have corresponding cutoff frequencies to separate the modulation signal in the GC microcoil from the signal at the second harmonic of the modulation frequency.

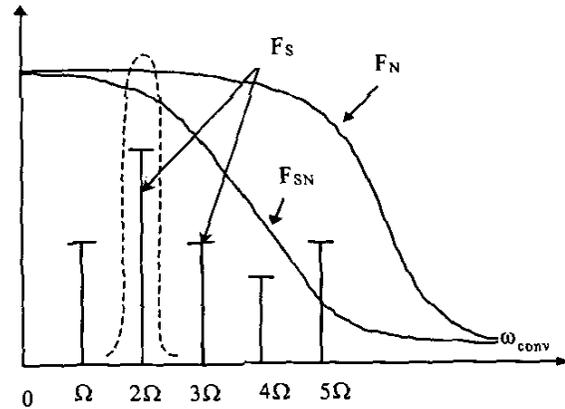


Fig. 5. Components of the spectrum of the converted additive sum "signal" + "noise".

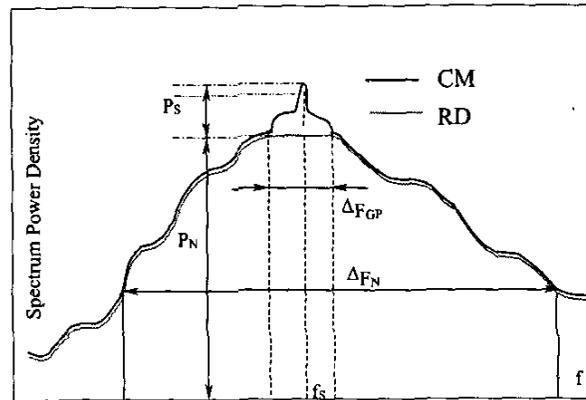


Fig. 6. Panoramic view of a wideband noise and a narrowband deterministic signal at the resonance detection and cross-multiplication regimes.

The experimental two-channel device allowed detecting reliably microwave narrowband deterministic signals, which power was up to 30 dB less than an integral power of the background noise signal. The GC of this experimental device was designed using a ferrite spherical resonator having a diameter of 0.5 mm. The resonator was made of monocrystalline YIG ferrite doped with Ca, Bi, and V ions, and had a comparatively low saturation magnetization of $4\pi M_S = 300$ Gauss (or $M_S = 23.9$ kA/m). The width of the ferrite resonance line at the level of -3 dB was about 2 MHz at frequencies above 300 MHz. The narrowband block, shown in Figure 3, was a frequency-selective RF amplifier with a pass band of 1 kHz tuned to the second harmonic of the modulation frequency. The frequency and the amplitude of modulation were optimal for getting the maximum voltage induced in the spiral coil of the GC at the second harmonic of modulation frequency. The second harmonic is used to separate the modulation signal in the microcoil from the induced voltage, and this is the most intense harmonic compared to the higher-order ones. According to studies of an optimum modulation regime [8,11], the normalized magnetic

field amplitude of modulation for the GC was $q=3.5$, and the relative modulation frequency was $p=0.8$. The plotter record of an additive sum of wideband noise and signal at the resonance detection and cross-multiplication regimes of the two-channel measuring device operation is presented in Fig.7. The input signal-to-noise ratio corresponding to this figure was -24.5 dB in the scanning band of 100 MHz. The measured amplitude of the detected signal was 0.4 mW. The spectrum envelope in the vicinity of the detected signal resembles the form of the second derivative of the FR resonance curve, or the form of the second harmonic of the FR magnetization versus detuning $\Psi_2(a)$. This specific form increases the reliability of the signal distinction from an inhomogeneity in the wideband random spectrum envelope.

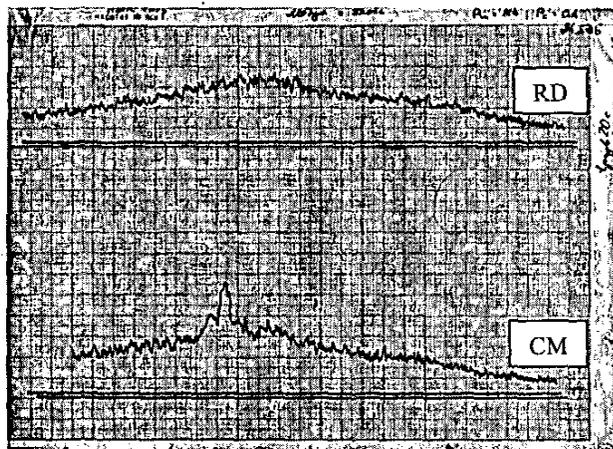


Fig.7. Plotter record of wideband noise and signal envelope at the resonance detection and cross-multiplication regimes of the TCMD operation.

It is important that the microwave narrowband signal instability does not lead to the necessity of the frequency-selective block pass-band widening. This is possible due to the non-heterodyne frequency conversion by a GC, since the frequency of a converted deterministic narrowband signal is independent of the microwave frequency carrier, but is determined only by a harmonic of a stable modulation frequency [2],

$$f_{conv} = n f_{mod}, \quad n = 2, 3, 4, \dots \quad (15)$$

Minimum possible pass-band of the narrowband amplifier is determined only by the condition non-distortion of the spectrum envelope at fast frequency sweeping at panoramic observation of the spectrum.

Design of the GC on base of prospective high-anisotropy monocrystalline hexagonal ferrites with high Q-factor increases the operation band of the proposed method and device to millimeter wave frequency range without necessity of using intense external magnetic fields [4].

III. CONCLUSION

Using stable non-linear resonance effects in high-quality monocrystalline ferrite resonators at their interaction with microwave random and deterministic signals, it is possible to provide both measuring of power parameters of wide-band intense noise and detecting narrow-band signals at the noise background. Essential increase of signal-to-noise ratio is achieved in the two-channel measuring device that uses gyromagnetic converter, at simultaneous narrowband amplifier and RF modulation switching on. Due to frequency-selectivity and non-heterodyne principle of frequency conversion, measuring devices that employ gyromagnetic converters have a number of advantages. They are free from parasitic channels of reception associated with heterodyne and intermodulation harmonics, resistant to microwave power overload, and can be used for visualization and measuring power (spectrum) parameters of radiations produced by high-power microwave devices.

REFERENCES

- [1] M.Y.Koledintseva, L.K.Mikhailovsky, A.A.Kitaitsev, "Advances of Gyromagnetic Electronics for EMC problems", in *Proc. 2000 IEEE Symp. Electromagn. Compat.*, Aug. 21-25, 2000, Washington, DC, vol.2, pp.773-778.
- [2] V.F.Balakov, V.A.Kartsev, A.A.Kitaitsev, N.I.Savchenko, "Application of gyromagnetic effects in ferrite monocrystals for electromagnetic signals parameters measurement", in *Proc. 5th Int. Conf. Microwave Ferrites*, 1980, Moscow, vol.3, pp. 86-99 (in Russian).
- [3] A.A.Kitaitsev, et al., "Panoramic measuring device for microwave signal power parameters", in *Transactions of Moscow Power Engineering Institute*, no. 241, Moscow: MPEI, 1991, pp. 40-47 (in Russian).
- [4] A.A.Kitaitsev, M.Y. Koledintseva, "Physical and technical bases of using ferromagnetic resonance in hexagonal ferrites for electromagnetic compatibility problems", *IEEE Trans. Electromagn. Compat.*, vol. 41, no. 1, Feb. 1999, pp.15-21.
- [5] A.G.Gurevich, G.A.Melkov, "Magnetic oscillations and waves", Moscow, Russia: Fizmatlit, 1994 (in Russian).
- [6] B.R.Levin, *Statistical communication theory and its applications*, translated from Russia, Moscow: Mir publishers, 1982.
- [7] M.Y.Koledintseva, A.A.Kitaitsev, V.A.Konkin, "High-power Microwave Wideband Random Signal Measurement and Narrowband Signal Detection Against the Noise Background", in *Proc. IEEE EMC Symp.* Montreal, Aug.13-17, 2001, vol. 2, pp. 1027-1029.
- [8] A.A.Kitaitsev, N.I.Savchenko, "Influence of the external magnetic field variation velocity on the oscillation of the longitudinal component of the ferrite magnetization at the FMR", in *Proc. Conf. Electron. Eng.*, Moscow, Russia, Apr. 1970, no. 925, pp. 77-79 (in Russian).
- [9] M.Y.Sizenova, "Phase spectrum computation for the ferrite longitudinal component of magnetization vector at alternating magnetizing field", *Trans. Moscow Power Eng. Institute "Gyromagnetic Devices and Antennas"*, no 99, Moscow: MPEI, 1986, pp. 23-28 (in Russian).
- [10] A.A.Kitaitsev, "Oscillation of magnetization when microwave signal and noise act on the magnetic detector", *Reports of Scientific Conf.*, Radio Engineering Section, Microwave Ferrite Radio Physics Subsection, Moscow, MPEI, 1969, pp. 36-39 (in Russian).
- [11] A.A.Kitaitsev, M.Y.Koledintseva, "Formation of the frequency selectivity curve of the gyromagnetic converter", *Transactions of Moscow Power Engineering Institute*, No 237, Moscow: MPEI, 1990, pp.38-44 (in Russian).